

NEDD4 E3 Ligase TR-FRET Kit

Cat. No. SBB-KF0056
Lot. No. 173050056



South Bay Bio

Introduction

South Bay Bio's NEDD4 E3 Ligase TR-FRET Kit provides a fast and sensitive method monitoring ubiquitin conjugation onto NEDD4 in solution, resulting from an enzymatic ubiquitin cascade without the need of running and staining an SDS gel. The kit enables continuous TR-FRET detection of ubiquitin chain formation onto NEDD4 in a real-time detection setup, or in an end-point configuration if desired. TR-FRET uses the extended fluorescence emission decay lifetimes typical of rare-earth lanthanides to impart a short time-delay between FRET donor excitation and emission. This delay provides a means to separate "true" signal from short-lived background fluorescence, and reduce interference from compound fluorescence and other assay artifacts.

The kit uses ubiquitin labeled with either Europium-Cryptate or Cyanine5 as FRET pair donor and acceptor fluorophores respectively, completely eliminating the need for antibody based detection setups. Enzymatic incorporation of the labeled ubiquitins into chains conjugated onto NEDD4 leads to an increase in fluorescence emission at 665 nm ($E_{m_{\text{acceptor}}}$) and decrease at emission wavelength 620 nm ($E_{m_{\text{donor}}}$).

Product Information

Quantity: 400 x 20 μL reactions
160 x 50 μL reactions

Kit Components:

- 100x UBA1.....100 μL
- 100x UBE2L3100 μL
- 100x NEDD4.....100 μL
- 100x TRF-Ubiquitin Mix100 μL
- 10x Reaction Buffer.....1 mL
- 10x Mg-ATP.....1 mL
- 384-well white low-volume microplate.....x 1

Storage: -80C, Avoid multiple freeze / thaw cycles. It is recommended to make aliquots of each reaction component upon first time use.

Setup Protocol


1) Mix components in this order: H₂O, 10x Reaction Buffer, 100x UBA1, 100x UBE2L3, 100x NEDD4, and 100x trf-Ubiquitin Mix to a final volume concentration of 1x. Wait to initiate the reaction(s) with 10x Mg-ATP until the plate is ready to read in plate reader.

Example setup for 1 mL final volume mixture:

- To 760 μL H₂O
Add... 100 μL 10x Reaction Buffer
10 μL 100x UBA1 (E1)
10 μL 100x UBE2L3 (E2)
10 μL 100x NEDD4 (E3)
10 μL 100x trf-Ubiquitin Mix

Initiate reaction(s) with final addition of 10% final volume, 10x Mg-ATP to each well. For negative control(s) wells substitute Mg-ATP with 1x Reaction Buffer.

It is recommended to pipette all the components (minus Mg-ATP), i.e. 90% of the final volume into each well first, then initiate the reactions with addition of the last 10% final volume of Mg-ATP or a solution of 1x Reaction Buffer for the negative control wells.

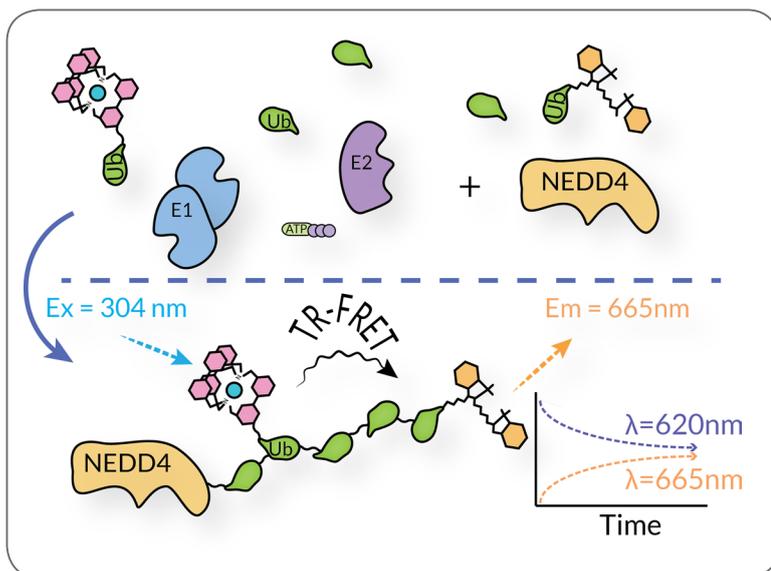

For Research Use Only, Not For Use In Humans.

www.southbaybio.com

Contact:
info@southbaybio.com

5941 Optical Ct, Suite 229
San Jose, CA 95138 USA

NEDD4 E3 Ligase TR-FRET Kit

Cat. No. SBB-KF0056
Lot. No. 173050056



South Bay Bio

2) Read 20-50µL reactions in a 384-well white low volume plate (supplied). You must use a plate-reader capable of taking top-read dual-channel TR-FRET measurements. Plate-readers tested with this kit include the Molecular Devices M5e Plate Reader and the PerkinElmer EnVision™ Multilabel Plate Reader. Plates can be read in either endpoint or continuous kinetic read mode.

Recommended Setting for Molecular Devices M5e


Channel 1: Excitation $\lambda = 304$ nm; Emission $\lambda = 620$ nm
Channel 2: Excitation $\lambda = 304$ nm; Emission $\lambda = 665$ nm
Delay Time = 50 μ s; Integration Time = 400 μ s
Cutoff $\lambda_1 = 570$ nm; Cutoff $\lambda_2 = 630$ nm

Recommended Setting for PerkinElmer EnVision

Top Mirror: LANCE/DELTA Dual Enhanced (#662)
Excitation Filter = UV2 (TRF) 320 nm (#111); Emission Filter₁ = APC 665 nm (#205); Emission Filter₂ = Europium 615 nm (#203); Delay Time = 50 μ s; Window Time = 400 μ s

Raw Data Output: Endpoint & Kinetic

Regardless of which type of readout that has been selected, the data must be collected on two channels; **Channel 1** measuring the emission signal of the donor cryptate at $\lambda_1=620$ nm, and **Channel 2** measuring the emission of the acceptor cyanine5 at $\lambda_2= 665$ nm. Both emission channels are required during data reduction to calculate percent signal : background and Z-primes.

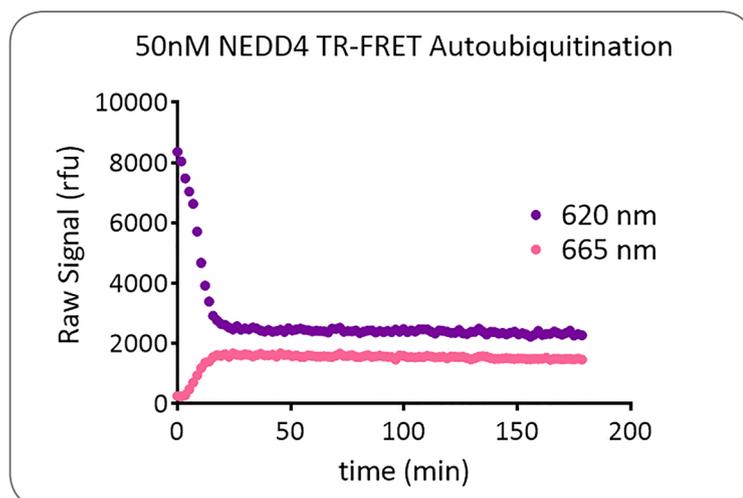

Raw Data Output: A single positive well continuously read in kinetic mode.

Data Reduction

Raw Signal: Aggregate TR-FRET signal detection is most typically quantified as the product of the ratio of acceptor to donor emission signal ($\lambda = 665$ nm/ $\lambda = 620$ nm), and a “convenience constant” ($\eta=10^4$):


$$\frac{\text{Emission}_2}{\text{Emission}_1} \left(\frac{\lambda = 665}{\lambda = 620} \right) \times 10^4 = \text{Raw Signal or } r(\text{Signal})$$

Specific Signal or Delta Signal: Subtracting the background raw-signal from the positive experimental-signal yields the “true” signal, also called the Delta Signal:

$$r(\text{Experimental}) - r(\text{Background}) = r(\text{Delta})$$

% Signal to Background: Different plates or experiments from different days of the same assay can be compared using the Signal to Background:

$$\frac{r(\text{Experimental}) - r(\text{Background})}{r(\text{Background})} \times 100\% = \frac{\text{Signal}}{\text{Background}} \%$$

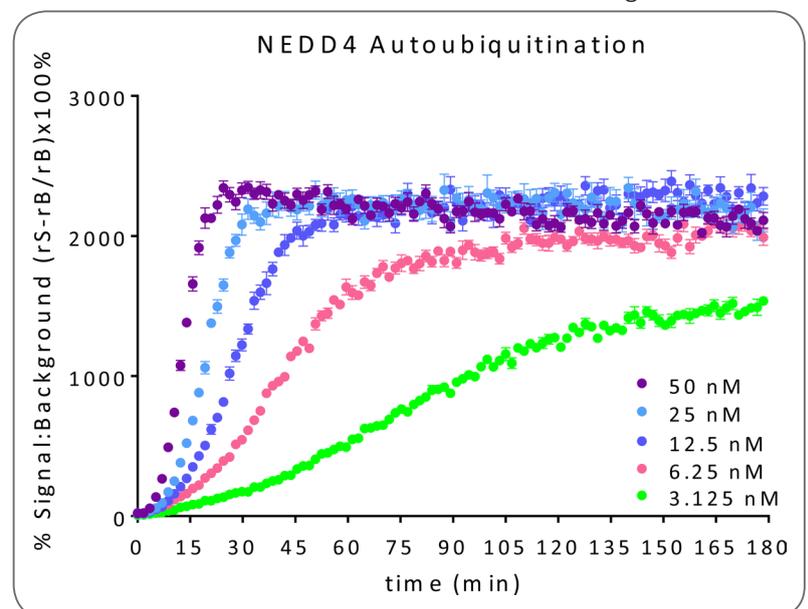

% Signal to Background of Continuous Real-Time TR-FRET NEDD4 titration (auto-ubiquitination): Serial dilutions of NEDD4 from 50 nM to 3.125 nM mixed with UBA1, UBE2L3, and trf-Ubiquitin mx. Reactions were initiated with addition of Mg-ATP.

For Research Use Only, Not For Use In Humans.

www.southbaybio.com

Contact:
info@southbaybio.com

5941 Optical Ct, Suite 229
San Jose, CA 95138 USA

NEDD4 E3 Ligase TR-FRET Kit

Cat. No. SBB-KF0056
Lot. No. 173050056



South Bay Bio

Z-Prime (Z'): Z-primes can be calculated by using the means and standard deviations of the positive and negative signal at each data-point over time.

$$\text{Estimated Z-prime} = 1 - \frac{3(\sigma_p + \sigma_n)}{|\mu_p - \mu_n|}$$


Where :

σ_p = standard deviation of the positive signal.

σ_n = standard deviation of the negative signal.

μ_p = mean of the positive signal.

μ_n = mean of the negative signal.

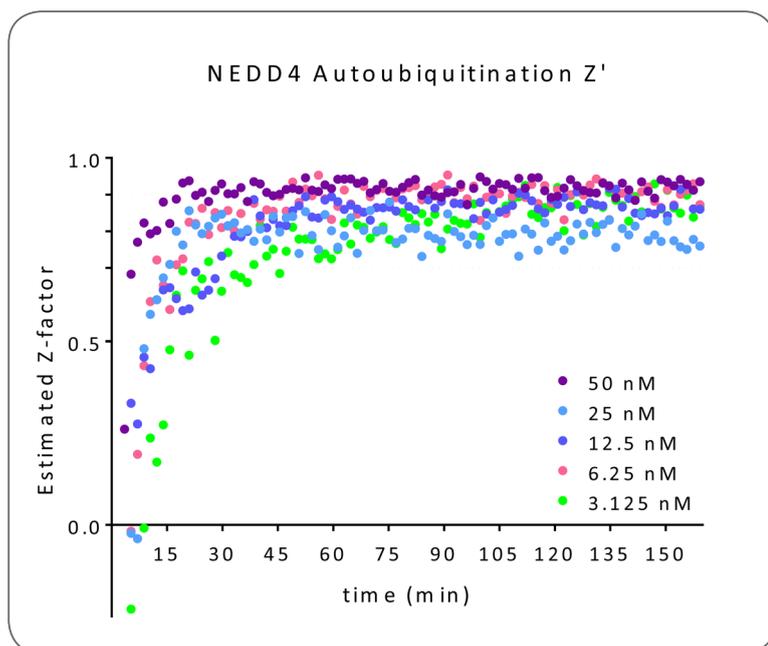

Estimated Z-primes of Continuous Real-Time TR-FRET MDM2 titration (auto-ubiquitination): Serial dilutions of NEDD4 from 50 nM to 3.125 nM mixed with UBA1, UBE2L3, and trf-Ubiquitin mix. Reactions were initiated with addition of Mg-ATP.

References

- 1) Magennis, S. W., Parsons, S., Pikramenou, Z., Corval, A., & Woollins, J. D. (1999). Imidodiphosphate ligands as antenna units in luminescent lanthanide complexes. *Chemical communications*, (1), 61-62.
- 2) Zheng, N., & Shabek, N. (2017). Ubiquitin Ligases: Structure, Function, and Regulation. *Annual Review of Biochemistry*, (O).

For Research Use Only, Not For Use In Humans.

www.southbaybio.com

Contact:
info@southbaybio.com

5941 Optical Ct, Suite 229
San Jose, CA 95138 USA